



QUICK REFERENCE GUIDE MR Q SUPINE (1)

SAFETY REQUIREMENTS




An appropriate safety glasses is required for all present persons when the System is in READY mode.

The MR Q has a built-in safety filter to protect the user

PRODUCT DESCRIPTION Energy Adjustment Control Inclinable Binocula Aiming Beam Intensity Control Illumination Towe Slitlamp LED Intensity Adjuster Magnification Adjustment Contro Laser Delivery Module LCD Control Unit Head Protection Foan Table Front Panel Joystick Electrical Column MASTER POWER SWITCH Wheels Electrical Wheel Brakes MAIN TABLE CONTROLS LASER SAFETY SWITCH ON/OFF TABLE UP/DOWN WHEELS LOCK/UNLOCK

ACCESSING THE MR Q



The laser does not have a KEY SWITCH, instead has a KEYPAD, a four number password is setup by the user. The Default Code is in the LASER KEY CABINET.


To unlock the laser the user must type the code followed by ------>



BEFORE USING THE LASER

User must calibrate the binoculars, to assure the laser focus and visualisation are on the same focal plane.

Position the laser head in the "Zeros" using the joystick



Switzerland

Finland

Slovenia

Meridian AG Bierigutstrasse 7 3608 Thun Meridian Medical Oy Elannotie 5 01510 Vantaa Meridian Medical d.o.o Plemljeva 8 1210 Ljubljana Distributor Information

OPHTHALMALOGIC / MERIDIAN Rick Behrens 0431 002 302






QUICK REFERENCE GUIDE MR Q SUPINE (2)

CONTROL PANEL

By pressing the icons, the setting is modified or reset.

FOR CAPSULOTOMIES & IRIDOTOMIES YAG TREATMENTS USE OFF-SET P100 or P200

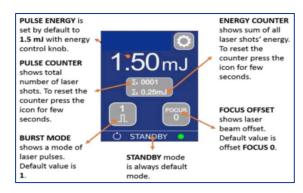

LASER CONTROLS



LASER LENS

Capsulotomy and iridotomy procedures often require the use of a laser lens, these are sourced independently by the user



SWITCH OFF

At The end of the case, press ON/OFF button and unlock wheels before unplugging the power

TROUBLESHOOTING

service@meridian.ch

 \rightarrow

DISPLAY	1	2	3	4	5
VIEW	1.50mJ	Device was not shut down property. Use CNVCF# button to continue.	WARNING Service due date 21.8.2017	WARNING Service required 21.8.2017	ERROR 12 Million Property and Marine and Million
STATUS	Normal operation	Fail operation	Normal operation	Normal operation	Fail operation
ACTION	Set required parameters for Ready mode.	Reset unit.	Press icon to confirm message.	Press icon to confirm message.	Reset unit and in case of remaining Error call service.

Switzerland

Meridian AG

3608 Thun

Bierigutstrasse 7

Finland

Meridian Medical Oy Elannotie 5 01510 Vantaa

Slovenia

Plemljeva 8

1210 Ljubljana

Meridian Medical d.o.o

Distributor Information

OPHTHALMALOGIC / MERIDIAN Rick Behrens 0431 002 302